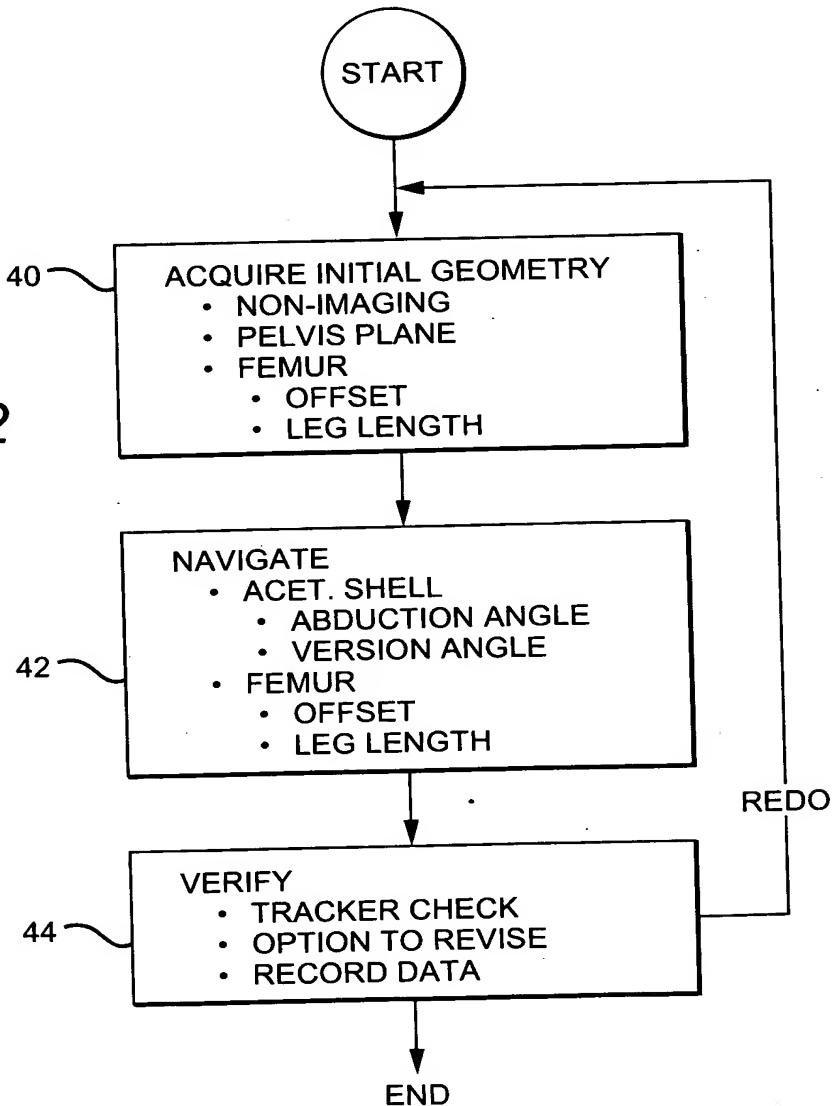
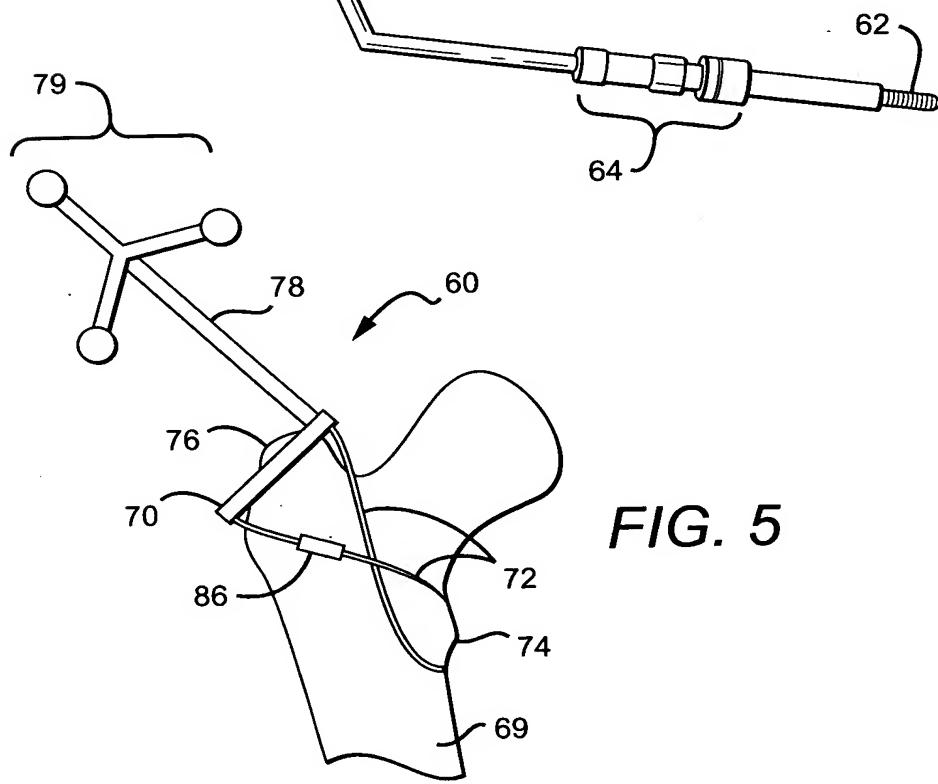
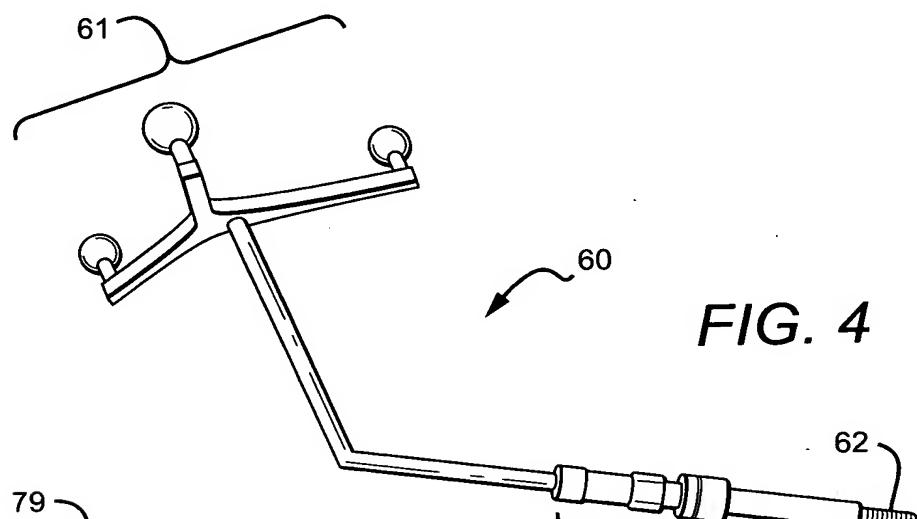
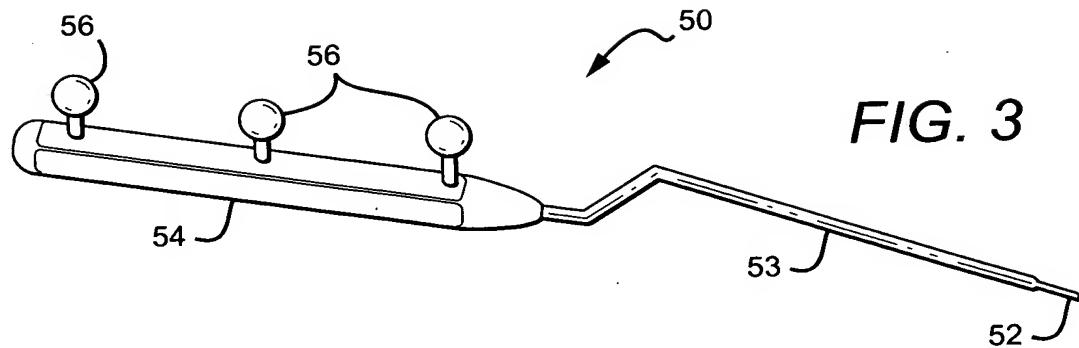


FIG. 1

FIG. 2





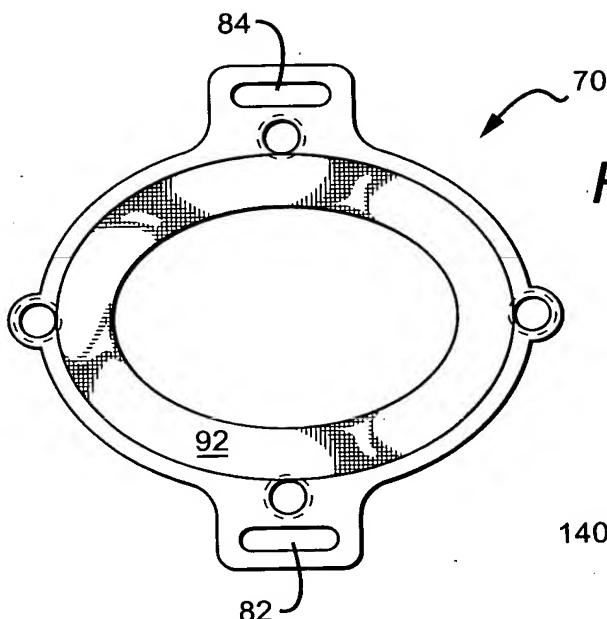


FIG. 6

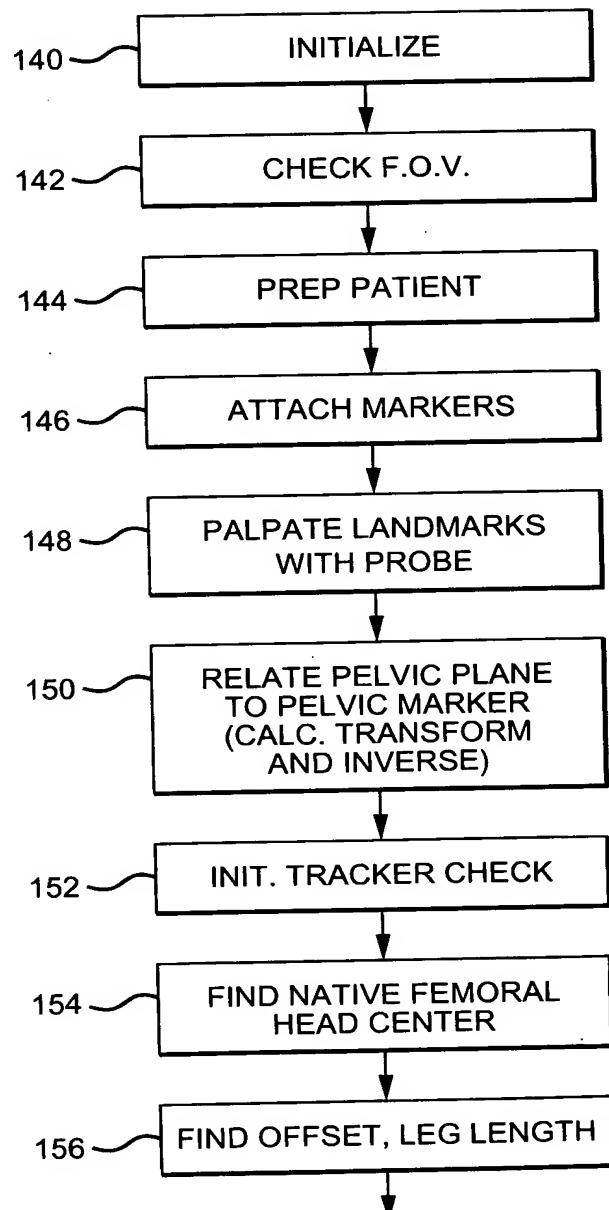
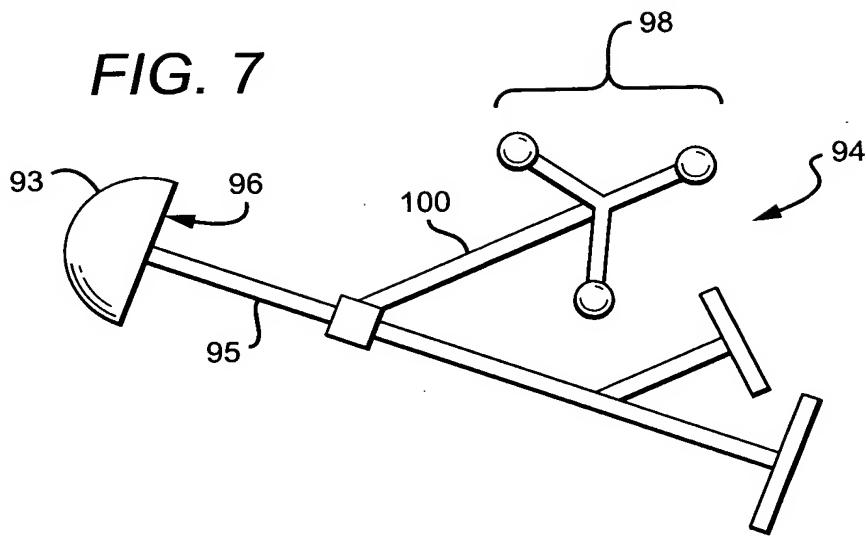


FIG. 8

FIG. 7

IMPACTOR POSITION

SHELL POSITION

LINER POSITION

HEAD CENTER CHANGE

LEG LENGTH CHANGE

HEAD OFFSET CHANGE

NOTE: RIGHT PEDAL SEND SUMMARY TO PRINTER, ALONG
WITH PATIENT DATA. SAVE ALL DATA TO FILE SPECIFIC TO
THIS RUN OF SOFTWARE. CHANGE SECURITY FLAG SO THAT
SAME CD CAN NOT BE USED TO START PROGRAM AGAIN.

FIG. 14

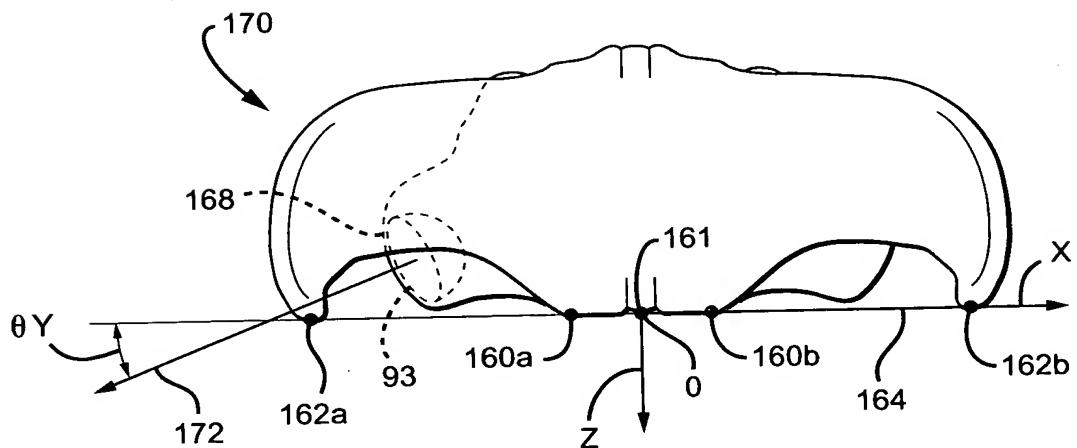
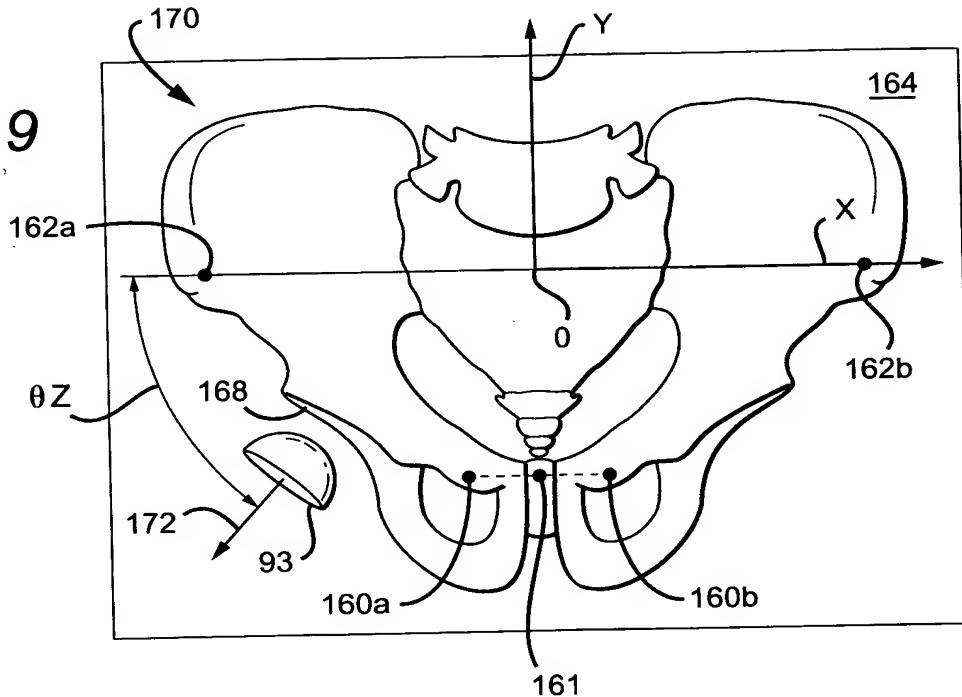
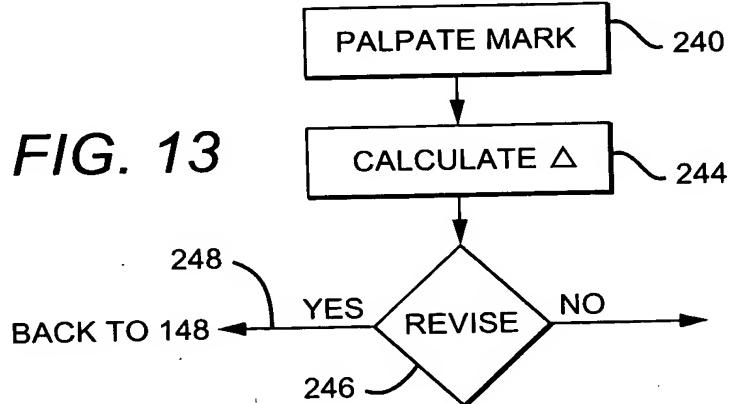
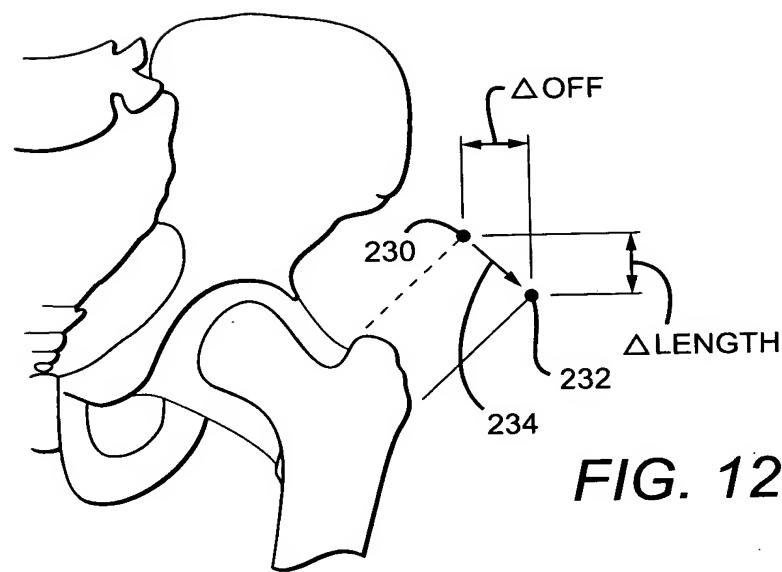
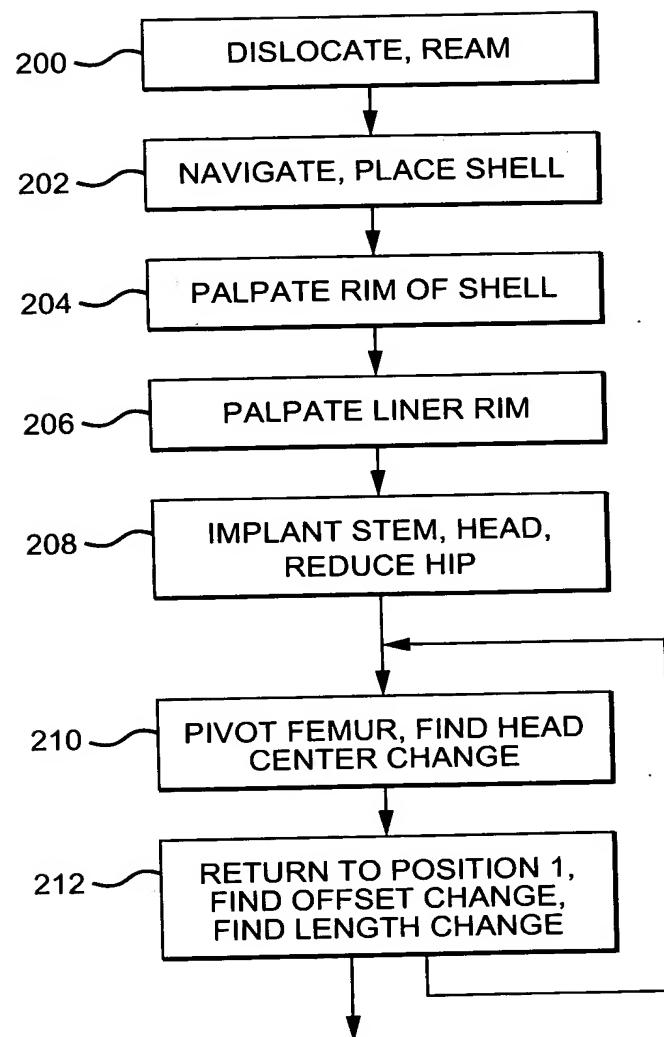
FIG. 9**FIG. 10****FIG. 13**

FIG. 11**FIG. 12**